

DIGITAL MICRO HARDNESS TESTERS



► MMT-X Feature

- •The new function deploy, color LCD touch panel.
- •The turret which mounted two indenter, four objective lenses.
- $\cdot \text{Testing}$ area of industry maximum class.
- ·Wide test force range.
- ·Line up in LCD model.
- \cdot 0.01 μ m measuring.(Magnification X200 \sim X1000)
- ·LED light source.





DIGITAL MICRO HARDNESS TESTERS

Operation

Color LCD touch panel

Visibility and operativity improve by color LCD touch panel. Equipped with the assist function that can identify the most suitable measurement condition.

(Correspondence model:X3,X7)

HV testing mode (Vickers Hardness)



HK testing mode (Knoop Hardness)



*Knoop indenter(option) is required.

Light-load brinell mode



Ball indenter(option) is required.

Xbar mode



This mode can display the mean and difference immediately.

Fracture toughness KC testing mode.




Cylindrical correction mode:



This mode can set spherical surface and cylindrical correction.

Assist function



This mode can identify the testing condition which is optimum is carried. The testing condition which is optimum can be comfirmed by satisfying 2 from 3 condition of thickness, haedness, test load.

Function

The turret which mounted two indenter, four objective lenses.



Two indenter and four objective lenses are realized following conventional stable loading mechanism. The measuring that reliability is high can be done in various test condition.

(All mode correspondence)

Measuring unit 0.01 μ m was realized by corresponding to high magnification of measuring total magnification 200×-1000×. (Correspondence model: X3.X7)

Operation

Line up in LCD model.

Clear specimen surface image magnified on TFT LCD monitor is displayed. Fatigue by the long operation is decreased. The integrated structure, there is no eye movement.

Because the Measurement knob is placed in the measurement

panel, you can significantly reduce the fatigue of working long

(Correspondence model: X3,X7)



Function

Testing area of industry maximum class.

By a new design.testing range of specimen height 120mm and specimen depth 160mm was secured.

(All mode correspondence)





MMT-X7

Digital model with auto turret.

Digital type

Min.scale: $0.01\mu m(200 \times \sim 1000 \times)$

Min measuring unit : $0.01 \mu m(200X\sim1000X)$

Touch panel type / Turret : Auto
Data output type / Dwell time : 5~99sec

MMT-X3

Digital model with touch panel.

Digital type

 $\mathbf{Min.scale}: 0.01\,\mu\mathrm{m}(200\times\!\sim\!1000\times)$

Min measuring unit : $0.01 \mu m (200 X \sim 1000 X)$

Touch panel type / Turret : Manual Data output type / Dwell time : $5\sim$ 99sec

MMT-X1

order made

Economy model of manual operation. Analog type

Specifications

Hardness Tester Model

Item / Model			MMT-X7 MMT-X3						MMT-X1					
Test force	Standard	Type A	49.03	98.07	24	5.2	490.3	980.	7	1961	2942	490	3 98	07mN
			5	10	2	25	50	100	Э	200	300	50	0 1	000gf
	Option	Туре В	9.807	29.42 49	9.03 9	98.07	245.2	490.3	980.7	1961	2942	4903	9807	19614 mN
	Option	l lybe p	1	3	5	10	25	50	100	200	300	500	1000	2000 gf
Loading	mechanism		Automatic loading and releasing method											
indenter	approach	speed	50μm/sec											
Dwe ll tim	ne		5~99sec 5~30sec											
Indenter							Standa	rd:1(H\	/),Opt	ion:2(H	V,HK)			
Objective	e lens		Standard:	2(50X,	10X %	in cas	se of AN	/IT-PS/F	S ser	ies : 50)X, 5X),	Option	Max.4	I(5X∼100X)
Eyepiece	lens		Standard10× option15×											
Total ma	gnification				Sta	andard	d(500X,	100X)	Corres	spondin	g50×~	-1000×		
	Max.measu	ring length	200μm											
Measuring microscope	Min.scale		0.01 µm(200X~1000X)						0.5 <i>µ</i> m					
(total 400×)	Min.measur	ing unit	0.01µm(200X~1000X)						0.1 <i>µ</i> m					
	Type		Electronic type							Mechanical type				
Light source		LED light source												
Turret				Auto		Manual								
LCD tou	ch panel		Color LCD touch panel -						-					
Testing I	mode		6 kinds of HV,HK,HBS,KC,Xbar,Cylindrical correction						-					
Data me	mory		999 data memory									-		
Hardnes	s conversior	1	Possible in compliance with SAE(J-417B),ASTM(E-140))			-		
OK/NG c	riteria		Judging to the results by setting Max. and Min.						-					
Statistic	al caluation		Max.value,Min.value,dispersion(R),mean value,converted value.											
Max. height of specimen			120mm											
Max. depth of specimen		160mm												
Data output		①Centronics(Dot printer output)												
		@RS232C(Output for PC),Possible to change to printer output												
Accuracy		According to JIS B7725 and ASTM E-384												
Photo booth		The photo booth can be installed in the body tube in the upper part of the main body at any time.												
Dimensions and weight			Main body only W250×D520×H530mm 35kg											
Power supply		Single phase AC100V~240 50/60Hz available for Export models												

TVL The 10.4inch TFT LCD monitor is attached. (All mode correspondence)



TV measuring device Set Model

LCD integrated model

Item / Model	MMT-X□-TVL				
CCD camera	1/2"CCD camera				
Monitor	10.4" TFT LCD				
Monitor magnification	≒ 1500×				
Min.scale	0.01 <i>µ</i> m				
Data display	Display on touch panel ※1				
Output	Monitor output(NTSC)				

 Item / Model
 MMT-X□-LCD

 CCD camera
 1/2"CMOS camera

 Monitor
 Tablet PC


 Monitor magnification
 ≒ 2000×

 Min.scale
 0.1 μm

 Data display
 Display on monitor

**Number of hardness tester is in a part of \square of a model name. LCD integrated model is only digital model.(X3,X7) *1 X1 do not have a data display function.

Automatic System

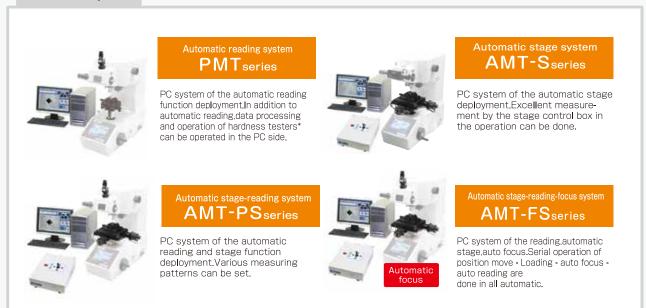


**Hardness tester models that can control is the only digital models.

Automatic System

Item / Model	PMT-X□	AMT-X□S	AMT-X□PS	AMT-X□FS				
Correspondence model	X1,X3,X7	X3,X7	X3,X7	X7				
Auto reading	0	_	0	0				
Data processing	0	0	0	0				
Auto stage	_	0	0	0				
Auto focus	_	_	_	0				
Stage control box	_	0	0	0				
PC	PC/AT convertible							
Monitor		19" TFT monitor						
OS	Windows XP professional SP3(Corresponding windows7 in the future.)							
Other	X-Y data input option	Corresponding exclusive fully automatic system *please consult						

*Number of hardness tester is in a part of \square of a model name.Please use an exclusive catalog on the details. *Windows is a registered trademark by Microsoft USA in USA and other countries.

Option

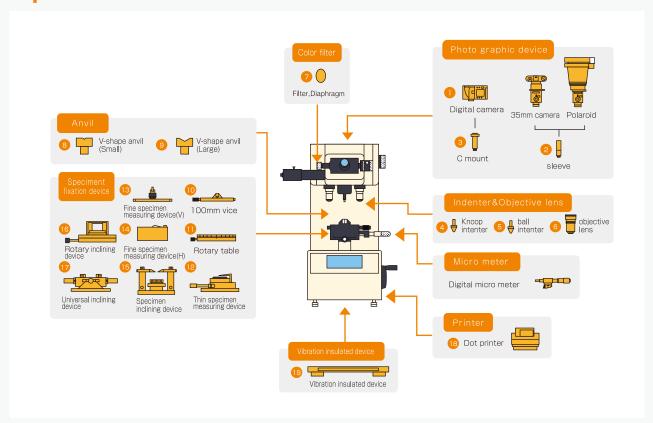

Factory Setting Option

ID Code	Item	Specification	Model	Note
LB	Test Force type	Type B(1 \sim 2000gf 12step)	All	Standard:Type A
AP	Test Force change device	Automatic change(Panel operation)	X3,X7	
ID	Indenter	Two simultaneous installation(HV,HK)	All	
T3,T4	Objective lens	T3:3 objective lens / T4:4 objective lens	All	Standard:2 lens
DM Micrometer		Digital micrometer	X3,X7	Displaying a coordinate value on touch panel & cable accessory

^{**}Specify the above option at the time of the order. An exchange becomes possible only in our company factory later.

Optional Accessories

Code No.	Item		Contents			
M201	Photographic device:Digital camera	1)	Nikon Microsystem(Digital camera,relay lens,accessory)			
M211	Camera sleeve	2	For polaroid camera or 35mm camera.			
M212	C mount	3	For digital camera or automatic system.			
M002	Knoop indenter(HK)	4	Effectively measures thin material.			
M003	Ball indenter(HB)	(5)	For light-load brinell test.(φ1mm cemented carbide steel ball)			
M071~075	Objective lens	6	100X(M071),40X(M072),50X(M080),20X(M073),10X(M074),5X(M075)			
M076	Eyepiece		15X			
M081	Color filter	7	φ20mm yellow,blue,red(standard:green)			
M082	Aperture diaphragm	7	1mm~6mm(1mm pitch,6 size)			
M020	V-shape anvil(Small)	8	For measuring the cylindrical surface together with vice. ϕ 2mm \sim ϕ 6mm			
M021	V-shape anvil(Large)	9	For measuring the cylindrical surface together with vice. ϕ 8mm \sim ϕ 50mm			
M012	Precision vice	10	Max. opening: 1 00mm			
M013	Rotary table	(1)	360° rotation. This table is usually on the micro test table with precision vice.			
M014	Thin specimen measuring device	12	Specimen thickness:0.05~5mm			
M015	Fine specimen measuring device(V)	13	Vertical type.Specimen diameter:0.1~4mm			
M016	Fine specimen measuring device(H)	14)	Horizontal type.Specimen diameter:0.5~4mm			
M017	Specimen inclining device	(15)	The mesuring surface always shows a horizontal level. Specimen height: 5~21 mm			
M018	Rotary inclining device	16	Specimen diameter: 1 inch, 1 1/4 inch, 1 1/2 inch select one size as you want			
M019	Universal inclining device	17	When the specimen is inclined or curved, this device is effective to get the correct level.			
C001	Dot printer	18	From CBM-910 I hardness tester adding up results to data output.			
M171~M175	Vibration insulated device	19	On the desk type(Rubber cushion type:M171,Manual air type:M172, Auto air type:M173,Compound mount type:M175),Desk type(M174)			
M102 Table for Knoop hardness number		r	For HK 5gf~50kgf			

Standard Accessories

Code No.	Item / Model	MMT-X7	MMT-X3	MMT-X1		
M031	Manual X-Y stage(Built in/Max.movement:25mm/Min scale:0.01mm)	1				
MO11	Precision vice(Max.opening:50mm)		1			
M061	Standard test block(700HMV0.2)	1				
M001	Diamond indenter		1			
M041	Measuring microscope:Electronic type	1		_		
M042	Measuring microscope:Mechanical type	- 1				
M080	Object lens 50×(Built in)		1			
M074	Object lens 10×(Built in)	1				
M111	Level adjusting leg	4				
M300	Level	1				
M094	Spare fuse(100~220V5A)	2				
C031	Power cord(3P 2.5m)	1				
M161	Machine cover	1				
_	Auxiliary tool kit	1				
_	Instruction manual(Basic&Application)	1				
_	Inspection sheet					
M101	Table for Vickers hardness number(5gf~50kgf)	_		1		

Data processing software

Hardness Data Communication Software(Option)

HARDCOM SERIES

Testing data are transmitted to Microsoft Excel directly.

Testing data can be managed if software is installed in the personal computer.



(Microsoft Excel is separately necessary.)

Connection method

Hardness meter output(RS232C)-PC input(RS232C or USB) *USB serial converters standard attachment · Corresponds to USB2.0

Data processing function

Testing data, test condition, statistics data and graph drawing are equipped.

Measurement position data can be input.

Testing position data are indicated by connecting a digital micro-meter.


(Digital micro-meter is separately necessary.)

Support an exclusive format.

The input part of the testing condition is freely revokable. Our company will produce it if there is hope by a special form. Code No. S001 Standard Software

Code No. S002 Software with the position data input function. Corresponding model:MMT-X3,X7 · VMT-X3,X7 · RMT-1,3

**RMT series does not have the functionality of a data entry position. OS:Windows2000,XP,Vista,7 Excel Version:corresponds up to 2010

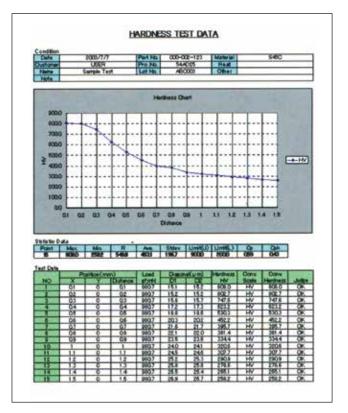

*Microsoft and Windows are registered trademark by Microsoft USA in USA and other details. *Contents of this brochure is April 2017. Specifications and appearance may change without notice.



120-19, Aza-Nanamagaridai, Toshima, Kawabe,

Akita-shi, Akita Pref, 019-2611, Japan

TEL.+81-18-882-4580 FAX.+81-18-882-4584

E-MAIL:support@matsuzawa-ht.com URL:http://www.matsuzawa-ht.com